

A large, vertical green bar occupies the lower half of the page. In the upper portion of this bar, there is a large white cross, which is a scaled-up version of the cross in the Triarc Medical logo.

**LABELLING SYSTEMS  
PRODUCT CATALOGUE**

FREE PHONE 0800 TRIARC (874272)  
[www.triarc.co.nz](http://www.triarc.co.nz)



## Welcome to the Triarc Medical Labelling System Product Catalogue

Triarc Medical has been driving innovation for over 30 years with our quality labels and dispensers for the medical environment worldwide.

We hope you enjoy browsing through this comprehensive product catalogue, which gives some insight into the range we do.

### The Company

Triarc Medical is a family-owned business which develops and supplies colour coded medical label systems into the medical and pharmaceutical environments worldwide. Triarc was established in the 1980's to produce a safe and convenient system for the labelling of Anaesthetic Drug Syringes. Triarc serves both local and international markets through its network of global distributors.

### The Products

Triarc Medical promotes patient safety and manufacture our anaesthetic syringe labels in accordance with the AS/NZS4375:1996 & ISO26825:2020 standards. We also produce labels for the Australian National Standard for 'User-applied Labelling of Injectable Medicines, Fluids and Lines'. These standards set out the requirements to reduce the risk of patient harm and help healthcare professionals. With over 10,000 pre-printed labels Triarc Medical has an extensive range to fulfil your needs. Triarc supply sterile label packs that are ready to use. We can customise your own selection of labels into individual pouches and sterilise them by Ethylene Oxide.

Triarc has developed a top quality label dispenser which is an integral part of the efficient, safe Triarc Medical Labelling System. The unique modular design gives you flexibility to configure your label bank exactly the way you need it to be.

### The Service

Our primary focus is to have quality products available when you require them. To this end, we are committed to stocking a large range of commonly used labels which are available by overnight courier. We also produce custom printed labels with short lead times

### The Care

Our Customer Service can help for any orders or enquiries you may have.



Phone: 0800 874 272  
TRIARC

or 06 878 5420



Email: [sales@triarc.co.nz](mailto:sales@triarc.co.nz)

Web: [www.triarc.co.nz](http://www.triarc.co.nz)

Quote

Within 24 hours

Proof

Within 48 hours

Custom  
Printed Item

Dispatch within 10 days  
from proof approval

Or

Stock Item

Despatch within 24 hours



# Label Dispensers



## THE PERFECT ANSWER TO A STICKY PROBLEM

The unique, modular design of the Triarc Medical Label Dispenser gives you more flexibility to configure your label bank exactly the way you need it to be.

- assorted widths
- fully enclosed
- easy reloading
- auto dispensing or tear & peel
- wall mounted or free standing
- horizontal or vertical stacking

Triarc Label Dispenser Sizes & Dimensions - TLD Range		
Code	Description	Dimensions (mm)
TLD15	DISPENSER - PLASTIC MODULAR 15MM WIDTH	128(l) x 134(h) x 20(w)
TLD25	DISPENSER - PLASTIC MODULAR 25MM WIDTH	128(l) x 134(h) x 30(w)
TLD35	DISPENSER - PLASTIC MODULAR 35MM WIDTH	128(l) x 134(h) x 40(w)
TLD45	DISPENSER - PLASTIC MODULAR 45MM WIDTH	128(l) x 134(h) x 50(w)
TLD55	DISPENSER - PLASTIC MODULAR 55MM WIDTH	128(l) x 134(h) x 60(w)
TLD65	DISPENSER - PLASTIC MODULAR 65MM WIDTH	128(l) x 134(h) x 70(w)
TLD75	DISPENSER - PLASTIC MODULAR 75MM WIDTH	128(l) x 134(h) x 80(w)
TLD85	DISPENSER - PLASTIC MODULAR 85MM WIDTH	128(l) x 134(h) x 90(w)
TLD105	DISPENSER - PLASTIC MODULAR 105MM WIDTH	128(l) x 134(h) x 110(w)
TLD115	DISPENSER - PLASTIC MODULAR 115MM WIDTH	128(l) x 134(h) x 120(w)
TLD125	DISPENSER - PLASTIC MODULAR 125MM WIDTH	128(l) x 134(h) x 130(w)

**Note: The backing paper width needs to be at least 1mm less, than the dispenser width**

For wider widths please contact us

Takes outer roll diameter up to 110mm


Auto Peel



Tear and Peel



### STACK MOUNT EXPAND

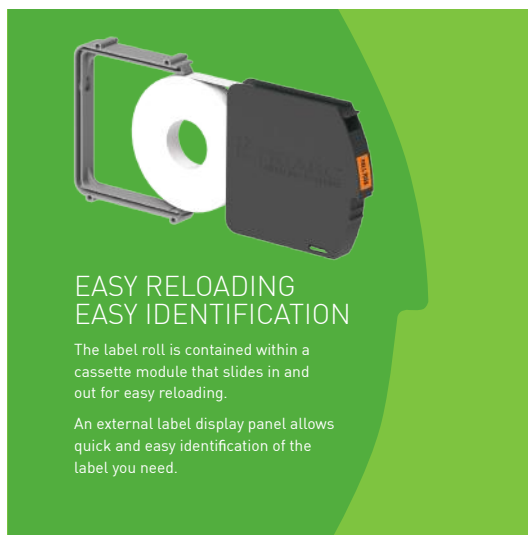

### EASY RELOADING EASY IDENTIFICATION

The label roll is contained within a cassette module that slides in and out for easy reloading.

An external label display panel allows quick and easy identification of the label you need.

## Anaesthetic Syringe Labels






**As per the AS/NZS 4375 : 1996 & ISO 26825 : 2020 Standards**  
 for User-applied labels for syringes containing drugs used during anaesthesia

Induction Agents	
<b>Thiopentone</b> mg/ml	R01
<b>Methohexitone</b> mg/ml	R02
<b>Propofol</b> mg/ml	R03
<b>Ketamine</b> mg/ml	R04
<b>Etomidate</b> mg/ml	R04A
<b>Perfantin</b> mg/ml	R04B

Muscle Relaxants	
<b>Atracurium</b> mg/ml	R06
<b>Pancuronium</b> mg/ml	R09
<b>Vecuronium</b> mg/ml	R10
<b>Suxamethonium</b> mg/ml	R11
<b>Muscle Relaxant</b>	R12
<b>Rocuronium</b> mg/ml	R12B

Muscle Relaxants	
<b>Mivacurium</b> mg/ml	R12C
<b>Cisatracurium</b> mg/ml	R12D

Relaxant Reversals	
 <b>Neostigmine</b> mg/ml	R13
 <b>Physostigmine</b> mg/ml	R27
 <b>Sugammadex</b> mg/ml	M0626

All codes are supplied as a roll of 500 labels



# As per the AS/NZS 4375 : 1996 & ISO 26825 : 2020 Standards

for User-applied labels for syringes containing drugs used during anaesthesia

Anticholinergic	
Atropine mg/ml	R14
Glycopyrrolate mg/ml	R15
Glycopyrronium mg/ml	R15N

Narcotic	
Alfentanil mcg/ml	R16
Narcotic	R16A
Fentanyl mcg/ml	R17
Morphine mg/ml	R18
Omnopon mg/ml	R19
Pethidine mg/ml	R20
Opioid	R20A
Papaverine mg/ml	R21A
Remifentanil mcg/ml	R21C

Narcotic	
Tramadol mg/ml	R21D
Physeptone mg/ml	R21E
Oxycodone mg/ml	R21F
Hydromorphone mg/ml	R21G
Fentanyl 1000ug / 50ml N/S	RAH17

Narcotic Antagonist	
Naloxone mg/ml	R22

Tranquillisers	
Diazepam mg/ml	R23
Midazolam mg/ml	R25
Phenytoin mg/ml	R25B

Tranquilliser Antagonist	
Flumazenil mg/ml	R26

Local Anaesthetics	
Bupivacaine %	R28
Lignocaine %	R29
Lidocaine %	R29N
Prilocaine %	R30
Ropivacaine %	R30A
Local Anaesthetic mg/ml	R30C
Levobupivacaine %	R30D
Bupivacaine (Adr) %	R31
Lignocaine (Adr) %	R32
Prilocaine (Adr) %	R33

Vasopressors	
Adrenaline	R34
Milrinone mg/ml	R34A

All codes are supplied as a roll of 500 labels



**As per the AS/NZS 4375 : 1996 & ISO 26825 : 2020 Standards**  
for User-applied labels for syringes containing drugs used during anaesthesia

Vasopressors	
Noradrenaline	R35
Ephedrine mg/ml	R36
Dopamine mg/ml	R37
Dobutamine mg/ml	R38
Metaraminol mg/ml	R39
Neosynephrine mg/ml	R39A
Phenylephrine mcg/ml	R39B
Vasopressor	R39C

Hypotensive Agents	
Dipyridamole mg/ml	R43C
Nimodipine mg/ml	R43D
Hydralazine	R43E
Hypotensive Agent	R43F
Clonidine mcg/ml	R43G

Anti-Arrhythmic	
Digoxin mcg/ml	R50
Isoprenaline mg/ml	R51
Verapamil mg/ml	R52
Adenosine mg/ml	R52A
Antiarrhythmic	R52B

Beta Blocker	
Labetalol mg/ml	R44
Metoprolol mg/ml	R45
Propranolol mg/ml	R46
Beta Blocker	R47
Esmolol mg/ml	R47A

Bronchodilators	
Aminophylline mg/ml	R53
Salbutamol mg/ml	R54

Hypotensive Agents	
Nitroprusside	R40
Nitroglycerin mg/ml	R41
Glyceryl Trinitrate mg/ml	R43A
Phentolamine mg/ml	R43B

Anti-Arrhythmic	
Amiodarone mg/ml	R48

Antiemetics	
Droperidol mg/ml	R24
Metoclopramide mg/ml	R55
Stemetil mg/ml	R56
Buscopan mg/ml	R56A

All codes are supplied as a roll of 500 labels



**As per the AS/NZS 4375 : 1996 & ISO 26825 : 2020 Standards**  
for User-applied labels for syringes containing drugs used during anaesthesia

Antiemetics	
Ondansetron mg/ml	R56B
Antiemetic	R56C
Tropisetron mg/ml	R56D
Cyclizine mg/ml	R56E
Granisetron mg/ml	R56F
Medetomidine	R56G

Electrolytes	
Calcium	R64A
KCl mmol/ml	R65
KH <sub>2</sub> PO <sub>4</sub>	R66A
Saline	R67
Mg SO <sub>4</sub>	R67A
Magnesium	R67B

Miscellaneous	
Fentanyl Midazolam	CM17/25
Morphine Midazolam	CM18/25
Neostigmine Atropine	HK13/14
Neostigmine Glycopyrrolate	HK13/15
WATER for inj.	M0001
Antibiotic	M0003
Antibiotic	M0003RP
Cephazolin	M0003C
_____mg/ml	M0004
	M0014
Dexamethasone mg/ml	M0044
Tranexamic Acid	M0087
Parecoxib	M0620

Ecobolics	
Ergometrine	R57
Oxytocin iu/ml	R58
Syntometrine	R59

Miscellaneous	
Insulin _____u	R60
Heparin iu/ml	R61
Heparin iu/ml	HW61
Hep. Saline iu/ml	R61A
Protamine mg/ml	R62
Frusemide mg/ml	R73

Electrolytes	
Calcium Chloride	R63
Calcium Gluconate	R64

All codes are supplied as a roll of 500 labels



# Sterile Label Packs

**Adrenaline**

SP0004 Vinyl/Waterproof  
1 label per pack

**Bleu Patente**

SP0008 Vinyl/Waterproof  
1 label per pack

**Methylene Blue**

SP0011 Vinyl/Waterproof  
1 label per pack

**CONTRAST**

SP0013 Vinyl/Waterproof  
1 label per pack

**Friars Balsam**

SP0014 Vinyl/Waterproof  
1 label per pack

**Antibiotic**

SP0015 Vinyl/Waterproof  
1 label per pack

**Hydrogen Peroxide**

SP0016 Vinyl/Waterproof  
1 label per pack

**Alcohol**

SP0018 Vinyl/Waterproof  
1 label per pack

**Papaverine**

SP0019 Vinyl/Waterproof  
1 label per pack

**PV Cream**

SP0020 Vinyl/Waterproof  
1 label per pack

**BIP Paste**

SP0021 Vinyl/Waterproof  
1 label per pack

SP0023 Vinyl/Waterproof  
2 labels per pack

**Botox**

SP0084 Vinyl/Waterproof  
3 labels per pack

**Ropivacaine**  
%

SP0039 Paper  
1 label per pack

**Bupivacaine**  
%

SP0040 Paper  
1 label per pack

**WATER for inj.**

SP0043 Paper  
1 label per pack

**CONTRAST**

SP0044 Paper  
1 label per pack

**Antibiotic**

SP0047 Paper  
1 label per pack

**Local Anaesthetic**  
mg/ml

SP0050 Paper  
1 label per pack

**Adrenaline**

SP0051 Paper  
1 label per pack

**Heparin**  
iu/ml

SP0052 Vinyl/Waterproof  
1 label per pack

**Saline**

SP0053 Vinyl/Waterproof  
1 label per pack

**Adrenaline**

SP0088 Vinyl/Waterproof  
3 labels per pack

**Glyceryl trinitrate**  
mg/ml

SP0115 Paper  
1 label per pack

SP0116 Paper  
1 label per pack

• Sterilised by ethylene oxide in individual pouches. • Customise your own selection of labels for your requirements.

Saline	Botox
Local	Local
Chlorsig	Maxitrol
Steroid	Antibiotics
Morphine	Adrenaline
Tranexamic acid	Water
Aqueous Prep	

SP0107 Vinyl/Waterproof  
14 labels per pack

B. S. S.	B. S. S.
ANTIBIOTIC	MIOTIC
STEROID	Local Anaesthetic mg/ml
CYTOTOXIC	MIDRIATRICS
HEAVY LIQUID	KENACORT
GAS	GAS
AIR	AIR

SP0108 Vinyl/Waterproof  
14 labels per pack





# Sterile Label Packs

<b>Contrast</b>	<b>Heparin</b> iu/ml	<b>Saline</b>	<b>Adrenaline</b>
<b>Bupivacaine</b> 0.5%	<b>Bupivacaine</b> 0.25%	<b>Bupivacaine 0.5%</b> <b>Adrenaline</b>	<b>Bupivacaine 0.25%</b> <b>Adrenaline</b>
<b>Ropivacaine</b> 0.2%	<b>Ropivacaine</b> 0.75%	<b>Ropivacaine</b> 1%	<b>Steroid</b>
<b>Tranexamic Acid</b>	<b>Gentamicin</b> mg/ml	<b>Cephazolin</b>	<b>Aqueous Betadine</b>

SP0117  
20 labels per pack

Paper

<b>Antiseptic</b>	<b>Antiseptic</b>
<b>Local Anaesthetic</b>	<b>Local Anaesthetic</b>
0.9% Sodium chloride	0.9% Sodium chloride
<b>Heparin</b>	<b>Contrast</b>
<b>Adrenaline</b>	<b>Steroid</b>
<b>Antibiotic</b>	<b>Miochol</b>
<b>BSS</b>	<b>WATER</b>

SP0069  
16 labels per pack

Vinyl/Waterproof

Medicine .....
Conc (units/mL) .....
Medicine .....
Conc (units/mL) .....
Medicine .....
Conc (units/mL) .....
Medicine .....
Conc (units/mL) .....
Medicine .....
Conc (units/mL) .....

SP0068  
5 labels per pack

Vinyl/Waterproof  
Removable Adhesive

- Sterilised by ethylene oxide in individual pouches.
- Customise your own selection of labels for your requirements.



# Colour Coding & Dot Labels

C02 WHITE	RC02 (REMOVABLE) WHITE	C03 LIGHT BLUE	C04 MID BLUE	C05 DARK BLUE		
C06 SALMON	C07 MID GREEN	C08 DARK GREEN	C09 LIGHT GREEN	C10 BRIGHT YELLOW		
C11 GOLDEN YELLOW	C14 ORANGE	C16 PURPLE	C17 MAGENTA	C18 MAUVE		
C19 PINK	C20 RED	C21 GREY	C22 VIOLET	C25 TEAL		
CR01 RADIANT RED	CR02 RADIANT ORANGE	CR03 RADIANT PINK	CR04 RADIANT GREEN	CR05 RADIANT YELLOW		
JCR02 RADIANT ORANGE 1000/BOX	JCR04 RADIANT GREEN 1000/BOX	RRP60X20 (REMOVABLE ADHESIVE) 500/BOX				
BKD14 BLACK 1050/BOX	BD14 BLUE 1050/BOX	GD14 GOLD 650/BOX	GRD14 GREEN 1050/BOX	LPD14 LIGHT PURPLE 1050/BOX	ND14 NAVY 1050/BOX	OD14 ORANGE 1050/BOX
PD14 PURPLE 1050/BOX	PID14 PINK 1050/BOX	RD14 RED 1050/BOX	WD14 WHITE 1200/BOX	YD14 YELLOW 1050/BOX	RGD14 RAD. GREEN 700/BOX	ROD14 RAD. ORANGE 700/BOX
BD24 500/BOX	GRD24 500/BOX	OD24 500/BOX	RD24 500/BOX	YD24 500/BOX		
RGD30 1000/BOX	ROD30 1000/BOX	RPD30 1000/BOX	RRD30 1000/BOX	RYD30 1000/BOX		

ALL 14mm AND 24mm DOTS ARE REMOVABLE ADHESIVE

ALL 30mm DOTS ARE PERMANENT ADHESIVE



## Slimline Food Labels

<b>VEGETARIAN</b> K01	<b>DIABETIC</b> K02	<b>LOW FAT</b> K03	<b>VEGAN</b> K06	<b>CHICKEN</b> K08
<b>LAMB</b> K09	<b>HAM</b> K10	<b>SALMON</b> K11	<b>BEEF</b> K12	<b>CORNBEEF</b> K13
<b>PORK</b> K16	<b>BACON</b> K19	<b>TUNA</b> K20	<b>SEAFOOD</b> K21	<b>SMOKED CHICKEN</b> K23
<b>SMOKED SALMON</b> K24	<b>DAIRY FREE</b> K25	<b>MINCE</b> K27	<b>MINCE &amp; CHEESE</b> K28	<b>EGG</b> K29
<b>CHEESE</b> K30	<b>GLUTEN FREE</b> K31	<b>CHEESE &amp; PINEAPPLE</b> K32	<b>CHEESE &amp; ONION</b> K33	<b>FOOD ALLERGY</b> K36

## Slimline Medical Labels

<b>ARTERIAL</b> ___/___/___ M0005	<b>M0014</b>	<b>M. R. S. A.</b> M0016	<b>CAUTION - DUPLICATE NAME</b> M0017	<b>ANAESTHETIC ALERT</b> M0018
<b>FALL RISK</b> M0019	<b>HEP. B POS.</b> M0029	<b>ALLERGY</b> M0034	<b>HEARING IMPAIRED</b> M0035	<b>ALERT</b> M0040
<b>ALERT</b> M0040RY	<b>DATE ___/___/___</b> M0041	<b>MAINTENANCE</b> M0042	<b>T.P.N.</b> M0043	<b>DIABETIC</b> M0048
<b>THROAT PACK</b> M0049	<b>Reversal</b> M0053	<b>CONTRAST</b> M0054	<b>CONTRAST</b> M0054BG	<b>CONTRAST</b> M0054RP
<b>DILUTE CONTRAST</b> M0055	<b>SIGHT IMPAIRED</b> M0059	<b>ADVERSE REACTION</b> M0066	<b>MEDIC ALERT</b> M0070	<b>SENSITIVITY</b> M0073
<b>IV Flush</b> M0079	<b>IV Flush</b> M0079RG	<b>DATE ___/___/___</b> <b>TIME ___/___/___</b> M0080	<b>DRUG ALERT</b> M0083	<b>C.V.P.</b> M0092
<b>Clonidine mcg/ml</b> M0095	<b>DIETITIAN</b> M0115	<b>Na Cl 0.9%</b> M0117	<b>PLEASE SIGN CONSENT</b> M0121	<b>OCCUPATIONAL THERAPY</b> M0123
<b>DIABETES NURSE</b> M0124	<b>ARTERIAL</b> M0125	<b>FORMALIN</b> M0126	<b>PHYSIO</b> M0128	<b>OCC THERAPY</b> M0129

All codes are supplied as a roll of 500 labels



# Slimline Medical Labels

<b>SLT</b> M0130	<b>NUTRITION</b> M0138	<b>DIETITIAN</b> M0139	<b>SOCIAL WORK</b> M0140	<b>NURSE</b> M0141
<b>PSYCHOLOGY</b> M0142	<b>PHYSIOTHERAPY</b> M0143	<b>SPEECH LANGUAGE THERAPY</b> M0144	<b>SOCIAL WORK</b> M0149	<b>MEDICAL</b> M0150
<b>NURSING</b> M0151	<b>SPEECH LANGUAGE THERAPY</b> M0153	<b>ACUTE PAIN SERVICE</b> M0157	<b>OCCUPATIONAL THERAPY</b> M0159	<b>DIETITIAN</b> M0170
<b>PAEDIATRIC</b> M0175	<b>PSYCHOLOGY</b> M0176	<b>INFECTION CONTROL</b> M0177	<b>N A S C</b> M0178	<b>GENTAMICIN</b> M0179
<b>KEFZOL</b> M0180	<b>DOUBLE STRENGTH</b> M0185	<b>BREASTFEEDING</b> M0202	<b>DISCHARGE PLANNING</b> M0208	<b>WOUND CARE</b> M0220
<b>PALLIATIVE CARE</b> M0223	<b>REHABILITATION</b> M0238	<b>MDT MEETING</b> M0239	<b>P.C.A.</b> M0255	<b>Consignment</b> M0259
<b>CONTACT PRECAUTIONS</b> M0265	<b>Heparin 5000u</b> M0274	<b>FORTIFIER ADDED</b> M0275	<b>SUNDAY</b> M0295	<b>MONDAY</b> M0296
<b>TUESDAY</b> M0297	<b>WEDNESDAY</b> M0298	<b>THURSDAY</b> M0299	<b>FRIDAY</b> M0300	<b>SATURDAY</b> M0301
<b>DIABETES</b> M0326	<b>FAMILY CONTACT</b> M0327	<b>FALL RISK</b> M0328	<b>CAUTION - DUPLICATE NAME</b> M0332	<b>Dynastat</b> M0344
<b>LACTATION CONSULTANT</b> M0368	<b>EPIDURAL</b> M0370	<b>WOUND SURVEILLANCE</b> M0385	<b>PAIN MANAGEMENT</b> M0401	<b>SPECIMEN TAKEN &amp; SENT</b> M0410
<b>OMNIPAQUE 300</b> M0417	<b>M.R.S.A. ALERT</b> M0418	<b>ALERT Patient on Anticoagulant</b> M0421	<b>OUT OF DATE</b> M0422	<b>DO NOT INJECT</b> M0466
<b>INSULIN ALERT</b> M0473	<b>FALL RISK</b> M0475	<b>Haloperidol mg/ml</b> M0476	<b>Spinal Morphine</b> M0481	<b>ALLERGY/ DRUG REACTION</b> M0484
<b>INPATIENT</b> M0502	<b>E. S. B. L. ALERT</b> M0509	<b>0.9% Saline</b> M0516	<b>PSYCHIATRIST</b> M0526	<b>NKDA</b> M0527

All codes are supplied as a roll of 500 labels



## Slimline Medical Labels

**CONSENT**

M0553

**RETURN TO PATIENT**

M0561

**PARACETAMOL**

M0565

**Infection Prevention & Control**

M0569

**infectious diseases ALERT**

M0585

**Dexmedetomidine**

M0667

**Vasopressin**

M0676

**EXPIRES IN JANUARY**

M0733

**EXPIRES IN FEBRUARY**

M0734

**EXPIRES IN MARCH**

M0735

**EXPIRES IN APRIL**

M0736

**EXPIRES IN MAY**

M0737

**EXPIRES IN JUNE**

M0738

**EXPIRES IN JULY**

M0739

**EXPIRES IN AUGUST**

M0740

**EXPIRES IN SEPTEMBER**

M0741

**EXPIRES IN OCTOBER**

M0742

**EXPIRES IN NOVEMBER**

M0743

**EXPIRES IN DECEMBER**

M0744

**CRUSHED MEDS**

M0781

## Slimline Endoscopy Labels

**ASCENDING**

OP0037

**CAECUM**

OP0050

**HEPATIC FLEXURE**

OP0136

**RECTO SIGMOID**

OP0198

**RECTUM**

OP0200

**RIGHT COLON**

OP0214

**SIGMOID**

OP0231

**SPLenic FLEXURE**

OP0237

**TERMINAL ILEUM**

OP0246

**TRANSVERSE**

OP0254

**GASTRIC BODY**

OP0363

**O. G. JUNCTION**

OP0364

**DUODENUM**

OP0365

**DESCENDING**

OP0366

**OESOPHAGUS**

OP0367

**ANTRUM**

OP0368

**LEFT COLON**

OP0369

**POLYP**

OP0487

**ASCENDING COLON**

OP0488

**TRANSVERSE COLON**

OP0490

**GASTRIC**

OP0492

**ANTRAL**

OP0839

**SIGMOID COLON**

OP0842

**BIOPSY**

OP1142

**COLAN**

OP1512

**ANTRUM**

OP0035

**BODY**

OP0042

**CAECUM**

OP0049

**DESCENDING**

OP0085

**DUODENUM**

OP0096

**OESOPHAGUS**

OP0183

**RECTUM**

OP0199

**SIGMOID**

OP0230

**SPLenic FLEXURE**

OP0236

**TRANSVERSE**

OP0253

**ASCENDING**

OP0275

**RIGHT COLON**

OP0461

**LEFT COLON**

OP0462

**RANDOM**

OP0463

**HEPATIC FLEXURE**

OP0514

**FUNDUS**

OP0519

**ANUS**

OP0520

**COLON**

OP0634

**GIARDIA**

OP0698

**DISACCH**

OP0699

All codes are supplied as a roll of 500 labels



# Pharmaceutical and Medical Labels

**PHARMACY**

M0284 500/ROLL

**PHARMACIST**

M0555 500/ROLL

**SECTION 29**  
COMPLETE ATTACHED  
PAPERWORK

M0348 500/ROLL

NEW PRESCRIPTION  
NEEDED. PLEASE  
CONSULT YOUR DOCTOR

M0222 500/ROLL

THIS IS THE SAME MEDICATION YOU  
HAVE BEEN GETTING, COLOUR, SIZE  
OR SHAPE MAY APPEAR DIFFERENT

M0513 500/ROLL

**SHAKE WELL  
BEFORE USE**

M0311 500/ROLL

**SECTION 29 MEDICINE**  
This product is unlicensed in NZ.  
Patient consents is required.

JG0477 500/ROLL

**SECTION 29 MEDICINE**  
Record Doctor and Patient  
names in register.

JG0478 500/BOX

**LIGHT  
SENSITIVE  
PRODUCT**

JG0504 1000/BOX

**REFRIGERATE**

JM0332 1000/BOX

**BROKEN PACK**

JM0203 1000/BOX

**USE FIRST  
SHORT DATED  
STOCK**

JM0286 500/BOX

**STORE IN THE  
FREEZER**

JG0235 250/BOX

**TAKE  
WITH  
FOOD**

JG0366 500/BOX

**Swallow Whole  
Do Not Crush or Chew**

JM0291 1000/BOX

**SHORT DATED  
STOCK**

JG0560 500/BOX

**CAUTION**  
Not to be taken

M0409 500/ROLL

DISPENSED BY | CHECKED BY

JM0367 500/BOX

**USE FIRST**

JG0087 500/BOX

**USE REGULARLY  
RINSE MOUTH  
AFTER USE**

JM0319 1000/BOX

**SHAKE THE BOTTLE**

M0411 500/ROLL

**CYTOTOXIC**  
Handle with Care

JG0428 500/BOX

**CYTOTOXIC**

M0428 500/ROLL

**CAUTION  
CYTOTOXIC  
DRUG**

JG0045 250/BOX

**CAUTION  
CYTOTOXIC**

JG0575 500/BOX

**HANDLE WITH CARE  
CYTOTOXIC  
DRUG**

JG0168 500/BOX

**Keep in Fridge  
Do Not Freeze**

JG0293 500/BOX

**SECTION 29 MEDICINE**

This product is unlicensed in NZ.  
Patient & Doctor consent  
is required.  
Patient & Doctor names  
are required by Pharmacy

JG0236 500/BOX

**CYTOTOXIC CYTOTOXIC**

JG0067 500/BOX

**FOR INTRAVENOUS USE ONLY  
FATAL IF ADMINISTERED BY  
OTHER ROUTES**

JG1148 500/BOX

**CAUTION**  
Product is NOT STERILE  
if packaging is open,  
damaged, or wet.  
Please check before using.

JG0021 250/BOX

**This product is  
SENSITIVE to LIGHT  
Keep in ORIGINAL packaging**

JG0390 500/BOX

**CONTROLLED DRUG -  
PLEASE STORE IN  
CONTROLLED DRUG SAFE**

JG0298 500/BOX

**TAKE WITH  
OR AFTER FOOD**

M0266 500/ROLL

**PHARMACIST**

JM0283 1000/BOX

**SWALLOW WHOLE  
DO NOT CRUSH OR CHEW**

JM0328 500/BOX

**TAKE WITH FOOD  
OR AFTER FOOD**

JM0329 500/BOX

**This medicine should be given  
to the patient at discharge.**

JG0570 500/BOX

**PROTECT FROM LIGHT**

JM0362 500/BOX



# Pharmaceutical and Medical Labels

**CAUTION  
CYTOTOXIC DRUG**

JG0170

500/BOX

THIS MEDICATION MAY NOT  
WORK AS INTENDED IF TAKEN  
WITH SOME OTHER MEDICINES  
ASK YOUR PHARMACIST

JG0714

500/BOX

**RESTRICTED  
DRUG**

M0470

500/BOX

This medicine may not work  
as intended if taken with  
some other medicines. Ask  
your pharmacist.

M0545

500/ROLL

**REFRIGERATED  
PRODUCT.**

Please refrigerate on  
arrival

JM0186

500/BOX

**PLEASE REFRIGERATE  
ON ARRIVAL  
DO NOT FREEZE**

JG0450

500/BOX

**PROTECT  
FROM LIGHT**

M0323

500/ROLL

THIS IS ONE OF  
SEVERAL CONTAINERS  
OF THE SAME MEDICINE

M0500

500/ROLL

**HYPERSENSITIVE TO:**

**PLEASE REFRIGERATE  
DO NOT FREEZE**

JG0449

500/BOX

**PLEASE REFRIGERATE  
ON ARRIVAL**

JG0022

500/ROLL

**STORE IN A CONTROLLED DRUG CUPBOARD**

JG0367

500/BOX

**STORE AT ROOM  
TEMPERATURE  
DO NOT REFRIGERATE**

JG0615

500/BOX

**SECTION 29 MEDICINE**  
Patient & Doctor names are  
required by Pharmacy

JG0668

250/BOX

**CAUTION NOT  
TO BE TAKEN**

JG0433

250/BOX

**NOT TO BE  
TAKEN**

M0069

500/ROLL

**CONTROLLED DRUG ( )**  
Keep in locked security cabinet  
Enter in register

JG0402

500/BOX

**PLEASE  
REFRIGERATE IMMEDIATELY  
ON ARRIVAL**

JG0313

500/BOX

**REMOVE CONTENTS &  
REFRIGERATE IMMEDIATELY  
ON ARRIVAL**

JG2058

500/BOX

THESE LABELS ARE AVAILABLE IN  
DIFFERENT COLOURS AND WITH  
YOUR PHARMACY NAME AND  
LOGO ON THEM

**DO NOT  
REFRIGERATE**

JM0146

500/BOX

3 Part Printer (Available in Thermal and Matt Material)

750/ROLL

BOX - Supplied with labels in a cardboard dispenser box. • ROLL - Supplied as labels on a roll only (Dispensers can be ordered separately).



# Jumbo Laboratory Labels / Jumbo Medical Labels

**DISCARD**

JG0436

100/BOX

**DO NOT DISCARD**

JG0437

100/BOX

**BIOLOGICAL HAZARD**

JG0217

500/BOX

**STERILE**

JG0211

500/BOX

**HANDLE WITH CARE HAZARDOUS DRUG**

JG0299

250/BOX

**STERILE**

JG0180

500/BOX

**FRESH SPECIMEN**

JG0102

500/BOX

**POISON**  
10% NEUTRAL BUFFERED FORMALIN HISTOPATHOLOGY

JG0289

500/BOX

**DECONTAMINATED**

JG0118

250/BOX

**10% FORMALIN**  
CAUTION CONTAINS FORMALDEHYDE TOXIC BY INHALATION AND IF SWALLOWED. IRRITATING TO THE EYES, RESPIRATORY SYSTEM AND SKIN. MAY CAUSE SENSITIZATION BY INHALATION OR SKIN CONTACT. RISK OR SERIOUS DAMAGE TO EYES. MAY CAUSE CANCER. REPEATED OR PROLONGED EXPOSURE INCREASES THE RISK.

JG0488

1000/BOX

**DATE \_\_\_\_\_**  
**TIME \_\_\_\_\_**  
**SIGNED \_\_\_\_\_**  
**I.V. SET UP**

JG0271

250/BOX



JM0266 250/BOX

**SOCIAL WORKER**

JM0193 500/BOX



JM0192 500/BOX



JG0393 500/BOX



JM0227 250/BOX

PATIENT'S NAME: .....  
BOTTLE NUMBER:..... DATE:.....  
DUE UP AT:..... DUE THRO:.....  
ADDITIVES:.....  
.....  
.....  
SIGNATURE:.....

JG0053

250/BOX

**SOCIAL WORKER**

JM0101

500/BOX

**ALERT**

JG0306

500/BOX

**SPINAL MORPHINE**

JG0431

500/BOX

**MEDICATION ADDED**

JG0081

500/BOX

**REPLACEMENT FLUIDS**    **REPLACEMENT FLUIDS**

JG0189

500/BOX

**SENSITIVITY ALERT**

JG0493

250/BOX

**EMERGENCY INSERTION**  
**REPLACE WITHIN 24 HRS**

JG0216RR

500/BOX





# Jumbo Medical Labels

BISHOP SCORE			
Date	Time		
Score	0	1	2
Position	Post	Mid	Ant
Consistency	Firm	Int	Soft
Length	3	2-1	<1
Dilatation	0	1-2	3
Station	-3	-2 -1	0
<b>Total</b>			
Cervidil	Given	Not Given	
Signature			

JG0583

500/ROLL

**COMMUNITY MENTAL HEALTH**

JM0260 500/BOX

**ARTERIAL LINE  
DO NOT INJECT**

JG0487 250/BOX

**TEMPORARILY OUT OF STOCK**

JM0258 (REMOVABLE ADHESIVE) 500/BOX

**RETURN TO PATIENT**

JG0124 250/BOX

**DRUG REACTION**

NAME OF DRUG

JG0028 250/ROLL

**PATIENT ON INSULIN**

See supplementary insulin chart

JG2044 500/BOX

**ALLERGY**

JG0001 500/ROLL

**PATIENT HAS OWN MEDICATION**

JG0119 250/BOX

**MEDICAL**

JM0173 1000/BOX

**PAIN MANAGEMENT SERVICES**

JG0552 500/ROLL

**NERVE BLOCK**

JG0542 500/ROLL

**EPIDURAL**

JG0005 500/ROLL

**REGIONAL CATHETER**

JG0007 500/ROLL

**EPIDURAL**

JG0826 500/ROLL

**ARTERIAL**

JG0143 500/ROLL

**VENOUS**

JG0144 500/ROLL

**P.C.A.**

JG0048 500/ROLL

**DOUBLE STRENGTH**

JG0147 500/ROLL

Surname: \_\_\_\_\_  
 Given Name: \_\_\_\_\_  
 NHI: \_\_\_\_\_ DOB: \_\_\_\_\_  
 Sign: \_\_\_\_\_ Date/Time: \_\_\_\_\_  
 Always label at the Bed-side

JG489 (PERFORATED BETWEEN LABELS) 250/ROLL

**BABY:**

DATE EXPRESSED: / /  
 TIME EXPRESSED: AM/PM

DATE DEFROSTED: / /  
 TIME DEFROSTED: AM/PM

JG0166 500/ROLL

**DO NOT DISCARD**

JG0042 250/BOX

**No Known Allergy**

JG0300 (GOLD) 250/BOX

**P.C.A. P.C.A.**

JG0073 500/BOX

**DRUG REACTION**

JG0092 250/BOX

**E.B.M.**

NAME: \_\_\_\_\_  
 DATE: / /  
 TIME: \_\_\_\_\_

JG0126 250/BOX



# Jumbo Medical Labels

**ANAESTHETIC  
HAZARD**

JG0037 500/BOX

**CYTOTOXIC CYTOTOXIC**

JG0067 500/BOX

**MAINTENANCE  
FLUIDS MAINTENANCE  
FLUIDS**

JG0068 500/BOX

**MORPHINE MORPHINE**

JG0069 500/BOX

**TPN TPN**

JG0070 500/BOX

**ATRACURIUM**  
\_\_\_\_\_ mg in \_\_\_\_\_ ml  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR06 500/ROLL

**CISATRACURIUM**  
\_\_\_\_\_ mg in \_\_\_\_\_ ml  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JRHK12D 500/ROLL

**FENTANYL**  
\_\_\_\_\_ mg in \_\_\_\_\_ ml NS  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR17 500/ROLL

**MORPHINE**  
\_\_\_\_\_ mg in \_\_\_\_\_ ml NS  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR18 500/ROLL

**PETHIDINE**  
\_\_\_\_\_ mg in \_\_\_\_\_ ml  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR20 500/ROLL

**MIDAZOLAM**  
\_\_\_\_\_ mg in \_\_\_\_\_ NS  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR25 500/ROLL

**ADRENALINE**  
\_\_\_\_\_ mg in \_\_\_\_\_ ml NS  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR34 500/ROLL

**NOR-ADRENALINE**  
\_\_\_\_\_ mg in \_\_\_\_\_ ml NS  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR35 500/ROLL

**DOPAMINE**  
\_\_\_\_\_ mg in \_\_\_\_\_ D5  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR37 500/ROLL

**DOBUTAMINE**  
\_\_\_\_\_ mg in \_\_\_\_\_ ml NS  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR38 500/ROLL

**PHENYLEPHRINE**  
\_\_\_\_\_ mg in \_\_\_\_\_ ml  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR39B 500/ROLL

**NITROGLYCERIN**  
\_\_\_\_\_ mg in \_\_\_\_\_ ml D5W  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR41 500/ROLL

**AMIODARONE**  
\_\_\_\_\_ mg in \_\_\_\_\_ ml D5W  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR48 500/ROLL

**ACTRAPID INSULIN**  
\_\_\_\_\_ U in \_\_\_\_\_ ml Gelofusine  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR60 500/ROLL

**HEPARIN**  
\_\_\_\_\_ U in \_\_\_\_\_ ml NS  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR61 500/ROLL

**KCl**  
\_\_\_\_\_ mmol in \_\_\_\_\_ ml  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JR65 500/ROLL

\_\_\_\_\_ mg in \_\_\_\_\_ ml \_\_\_\_\_  
at \_\_\_\_\_ /

JG0013 500/ROLL

**PROPOFOL**  
\_\_\_\_\_ mg in \_\_\_\_\_ ml  
Date/Time \_\_\_\_\_  
Added/Checked by \_\_\_\_\_

JRHK03 500/ROLL



# Jumbo Medical Labels

**MORPHINE  
MIDAZOLAM**

JG0140

500/ROLL

**INSULIN**

JG0142

500/ROLL

**PROTAMINE**

JG0521

500/ROLL

**ADRENALINE**

JG0133

500/ROLL

**MILRINONE**

JG0198

500/ROLL

**NORADRENALINE**

JG0134

500/ROLL

**DOPAMINE**

JG0135

500/ROLL

**DOBUTAMINE**

JG0136

500/ROLL

**PHENYLEPHRINE**

JG0520

500/ROLL

**VASOPRESSIN**

JG0199

500/ROLL

**NIPRIDE**

JG0137

500/ROLL

**TRIDIL**

JG0138

500/ROLL

**GTN**

JG0515

500/ROLL

**MORPHINE**

JG0139

500/ROLL

**ARTERIAL      ARTERIAL**

JG0114

500/BOX

**C.V.P.**

**C.V.P.**

JG0115

500/BOX

**ARTERIAL**

JG0161

500/BOX

**HAZARDOUS  
SUBSTANCE**

JG0336

250/BOX

**C.V.P.**

JG0162

500/BOX

**HAZARD  
ALERT**

JG0016

500/ROLL

**IV CANNULATION**

Date: \_\_\_\_\_ Time: \_\_\_\_\_

Inserted by: \_\_\_\_\_

Attempts: \_\_\_\_\_ Gauge: \_\_\_\_\_

Insertion Site: \_\_\_\_\_

Dressing: \_\_\_\_\_

Reason: \_\_\_\_\_

JG0157

100/BOX

**MEDICINE ADDED**

MEDICINE

AMOUNT

ADDED BY

DATE

TIME

JG0054

500/BOX

**ALLERGY**

JG0247

1000/BOX

**TUBINGS CHANGE DUE :**

DATE: / /

JG0036

500/BOX

**MEDICATION ADDED**

DRUG

AMOUNT

ADDED BY

DATE

Time

THIS LABEL MUST BE AFFIXED TO ALL INFUSION FLUIDS CONTAINING ADDITIONAL MEDICATION.

JG0027

500/BOX

**MEDICATION  
ADDED**

Name

Pt Number

Drug/Dose

Added by

Date

Time

JG0280

500/BOX

**MEDICATION ADDED**

Name

NHI

Drug

Amount

Added by

Date

Checked

Time

JG0365

500/BOX



# Jumbo Medical Labels

**INTRATHECAL MORPHINE**

DATE: TIME:

ADMINISTERED BY:

MONITORING REQUIRED FOR 24 HOURS

JG0619

500/BOX

**LATEX ALLERGY**

JG0125

500/BOX

**LATEX PRECAUTION**

JG0148

500/BOX

**HEPARIN**

\_\_\_\_\_ U in \_\_\_\_\_ ml NS

Date/Time \_\_\_\_\_

Added/Checked by \_\_\_\_\_

JRHW61

250/BOX

**ALLERGY**

DRUG:

JG0564

500/ROLL

**EPIDURAL EPIDURAL**

JG0485

500/BOX

**EPIDURAL**

JG0026

500/ROLL

**ALLERGIC TO**

JG0080

100/BOX

**URGENT**

JM0004

500/BOX

**THROAT PACK**

JG0034

500/ROLL

**DENTURES**

JG0225

250/BOX

**BSS 500mls**

Medication Added

Heparin 0.8mls 800 units

Adrenaline 1 in 1000 0.25mls

JG0812

500/BOX

**PLEASE NOTE  
CHANGE  
OF APPOINTMENT**



JM0085

250/BOX

**PLEASE RETURN TO  
THEATRE**

JG0018

500/ROLL

**FRAGILE**

JM0218

500/BOX

**ALLERGY**

JG0353

500/BOX

**MEDICATION  
ADDED**

JG0164

250/BOX

**ALLERGY**

DRUG:

REACTION:

JG0078

500/BOX

**ALERT  
DOSAGE**

JG0088

250/BOX

**LINE COMMENCED :**

DATE: / /

JG0323

250/BOX

**HEPARIN/GENTAMICIN LOCK**

Heparin 5,000u/ml)

Gentamicin 5mg ) in \_\_\_\_\_ mls

Date/Time \_\_\_\_\_

Added/Checked by \_\_\_\_\_

JG1195

250/BOX

**Body  
part/tissue  
to be returned  
to patient**

JM0719

250/BOX



JG0096

500/BOX

**INFECTION CONTROL**

JG0121

500/BOX



**WARNING  
ARTERIAL LINE  
DO NOT INJECT**

JG0154

500/BOX

**OBSTETRIC  
NOTES**

JG0075

500/BOX

**IRRIGATION FLUIDS**

JG0091

1000/ROLL

**WOUND  
CATHETER**

JG0813

500/BOX

**CAUTION  
DUPLICATE NAME**

JG0113

500/BOX

**EPIDURAL EPIDURAL**

JG0311

500/BOX

**NAME OF SET:**

**DATE OF OPERATION:**

**SURGEON:**

**PATIENT NAME:**

**PACKED BY:**

**NUMBER OF CRATES:**

JG0581RR (RAD. RED) JG0581RO (RAD. ORANGE) JG0581RP (RAD. PINK)  
JG0581RG (RAD. GREEN) JG0581RY (RAD. YELLOW) JG0581BW (WHITE)

500/ROLL



JM0257

500/BOX

**infectious  
diseases  
ALERT**

JG0122

250/BOX

**ACC**

JM0655

500/BOX

**L.A.**

**L.A.**

JG0407

500/BOX

**For Intravenous Use Only -  
Fatal if given by other routes**

JG0807

500/BOX

**10% FORMALIN  
TOXIC, ECOTOXIC**

JG0739

500/BOX

**M.D.R.O**

JG0757

500/BOX

**DENTURES**

JG0223

250/BOX

**E.S.B.L.  
ALERT**

JG0729

500/BOX



JM0300

500/BOX



## Intrathecal Morphine

This patient has received Intrathecal (spinal) Morphine O. \_\_\_\_\_ mg for pain control. Please monitor vital signs, especially sedation and respiratory care for 24 hours as per laminated "Intrathecal Morphine management sheet"  
 Date \_\_\_\_\_ Time of administration \_\_\_\_\_ hrs

JG0439

500/BOX

## CHECK PATIENT DETAILS

There is Another Patient with Similar or Same Name

JM0237

250/BOX

### SPECIAL NOTE

THERE IS ANOTHER PATIENT WITH THE SAME OR SIMILAR NAME  
**CHECK!**

JM0527

500/BOX

# INFECTIOUS

JG0248

250/BOX

# THROAT PACK

JG0030

250/ROLL

# EPIDURAL

JG0214

500/BOX

## DRUG ALLERGY

JG0074

500/BOX

## INFECTION PRECAUTIONS

JG0406

500/BOX

## STARTED

Date: \_\_\_\_\_ Time: \_\_\_\_\_

JG2106

500/BOX

INSERTION DATE \_\_\_\_\_

INSERTED BY \_\_\_\_\_

JG0020

250/BOX

## ADDITIVE LABEL

Patient Name: \_\_\_\_\_

Fluid: \_\_\_\_\_ Unit No.: \_\_\_\_\_

Drug Added: \_\_\_\_\_ Dose: \_\_\_\_\_

Date and Time Prepared: \_\_\_\_\_

Prepared by: \_\_\_\_\_ Checked by: \_\_\_\_\_

JG0270

250/BOX

## Rh neg MOTHER

CORD BLOOD TAKEN  YES  NO

MOTHERS BLOOD TAKEN  YES  NO

ANTI D GIVEN  YES  NO

JG0041

250/BOX

INSERTION DATE \_\_\_\_\_  
 INSERTION TIME \_\_\_\_\_  
 INSERTED BY \_\_\_\_\_

JG0031

250/BOX

## ORAL DRUGS

JG0035

500/BOX

P+NAME .....  
 DILUTANT .....  
 DRUG ..... AMOUNT .....  
 PREPARED DATE ..... TIME .....  
 PREPARED BY .....  
 CHECKED BY .....

JG0064

500/BOX

## PERIPHERAL IV CATHETER

Insertion Site: .....

Catheter Gauge: .....

Date: ..... Time: .....

Inserted by: .....

Date removed: .....

JG0110

250/BOX

DATE INSERTED \_\_\_\_\_

REPLACEMENT DATE \_\_\_\_\_

JG0019

250/ROLL

CRUSHED MEDICATION  
 Dr sign \_\_\_\_\_

JG0783

500/BOX

SPECIMEN TO BE RETURNED TO PATIENT

PATHOLOGIST	SENT
-------------	------

JG0317

500/BOX

POLYP \_\_\_\_\_

JG0268

500/BOX

## MAINTENANCE

JG0146

500/ROLL



# Jumbo Medical Labels

INSERTED BY \_\_\_\_\_  
 DATE OF INSERTION \_\_\_\_\_  
 REPLACEMENT DATE \_\_\_\_\_

JG0188 250/BOX

**ALERT  
 NOTIFICATION**

-----  
 -----

JG0278 250/BOX

**ALLERGY**

-----  
 -----

JG0284 500/BOX

**OUT OF FREEZER  
 DATE:  
 TIME:**

JG0781 500/BOX

Amber / Screening (Please circle)  
**ESBL**  
**VRE**  
**MRSA**  
 State reason for screening-

JG0912 500/BOX

**TISSUE TO BE RETURNED TO PATIENT**

Authorised by: \_\_\_\_\_ Sent to: \_\_\_\_\_  
 Sent by: \_\_\_\_\_ Date sent: \_\_\_\_\_

JG0556 500/ROLL

**ACC**

JM0152 500/BOX

SECURITY SEAL SECURITY SEAL SECURITY SEAL SECURITY SEAL

JG1634 250/BOX

**HEP.B + VE**

JG0014 500/ROLL

**Discharge Checklist**

Discharge Date: \_\_\_\_\_  
 Speciality: \_\_\_\_\_  
 Required for: \_\_\_\_\_  
 Date Required: \_\_\_\_\_

Discharge summary  
 Stacked  
 Coding summary  
 Letter typed / signed  
 Coded cc3078

JG0252 (REMOVABLE ADHESIVE) 100/BOX

**LINE CHANGE DUE :**  
 DATE: / /

JG0029 500/BOX

**LINE COMMENCED :**  
 DATE: / /

JG0163 250/BOX

**LINE CHANGED ON:**  
 DATE \_\_\_ / \_\_\_ / \_\_\_  
 TIME \_\_\_\_\_

JG0337 500/BOX

 **I'VE BEEN CLEANED**  
 DATE / /

JM0123 (REMOVABLE ADHESIVE) 500/BOX

**SURNAME:** \_\_\_\_\_  
**NHI NUMBER:** \_\_\_\_\_  
 /24 H BAG  
 DATE: \_\_\_\_\_

\_\_\_\_\_

\_\_\_\_\_

\_\_\_\_\_

\_\_\_\_\_

JG0108 200/ROLL

**Spinal / Epidural  
 Morphine**

JG0210 500/BOX

**EPIDURAL**

JHK0026 500/ROLL

**PLEASE CONFIRM THIS  
 APPOINTMENT**   
**PH:**

JG0046 500/BOX

HAVE YOUR PHONE NUMBER INCLUDED AT NO EXTRA COST

**IV CANNULA**

Insertion Date: / /  
 Time: AM/PM Gauge:  
 Print Name: \_\_\_\_\_ Sig: \_\_\_\_\_  
 Removal Date: / /

JG0046 500/ROLL

**IV CANNULA**

Insertion Date: / / Time: AM/PM  
 Gauge: \_\_\_\_\_ Site: \_\_\_\_\_  
 Print Name: \_\_\_\_\_ SIG: \_\_\_\_\_  
 Removal Date: / / JG490

JG0490 500/ROLL

**CAUTION  
 DUPLICATE  
 NAME**

JG0167 100/BOX

**P.C.A.**

JG0076 500/BOX



# Jumbo Medical Labels

## HEPARIN

JG0421

500/ROLL

## PCA

JG0331

## PCA

500/BOX

## CERVICAL SCREENING

JG0867

250/BOX

### HYPER-SENSITIVITY

JG0246

500/BOX

## RETURN TO PATIENT

JM0117

500/BOX



### CORROSIVE

Contains concentrated HCl acid  
Avoid contact with skin  
- will burn  
Do not void directly into bottle  
- may result in injury!!!  
If spillage/splashing occurs  
wash immediately with  
copious amounts of water

### URINARY CATHETER INSERTION

Date \_\_\_\_\_ Inserted By \_\_\_\_\_  
Batch no. \_\_\_\_\_ Expiry date \_\_\_\_\_  
Site: Supra Pubic  Urethral   
Type: All Silicone  Silicone coated   
Latex  Hydrogel  Banana   
Size of Catheter \_\_\_\_\_ FG H<sub>2</sub>O \_\_\_\_\_ ml

JG0618

250/BOX

JG0810

500/BOX

## SAFE WARMING

REMOVE BY: \_\_\_\_\_  
(DATE)

## SPECIAL DIET

JM0238

500/BOX

## CV LINE

JG0077

500/BOX

## ALERT

JG0200

500/BOX

JM0210

500/BOX

## HAVE YOU CHECKED FOR ANTICOAGULANT

JG0897

500/BOX

### The 5 R's

- Right Patient
- Right Drug
- Right Dose
- Right Route
- Right Time

Name: \_\_\_\_\_  
Signature: \_\_\_\_\_  
Time & Date: \_\_\_\_\_  
Drug Exp.: \_\_\_\_\_

JG0220

500/ROLL

## RETURN BODY PARTS

JG0441

500/BOX

## GROUP B STREP

JG0568

500/BOX

## RETURN TO PATIENT BODY PARTS

JG0599

500/BOX

### Infusion / Medication

Patients Name: \_\_\_\_\_  
NHI: \_\_\_\_\_  
Date: \_\_\_\_\_  
Time: \_\_\_\_\_

JG0908

500/BOX

## ALERT SKIN TEAR RISK

JG0690

500/BOX

### WARMED IV FLUIDS

**MUST** be used within 14 days once placed in the warmer

Expiry Date: \_\_\_\_\_

DISCARD AFTER EXPIRY DATE

JG0608

500/BOX

Hearing Screen



PASS

JM0443

500/BOX





# National Recommendation Labels

## For IntraTHECAL Use Only

Patient .....  
ID ..... DOB .....

Medicine/s	Amount (units)	÷	Volume (mL)	=	Conc (units/mL)
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....

Diluent .....  
Date ..... Prepared by .....  
Time ..... Checked by .....

JG1166

500/BOX

## For IntraTHECAL Use Only

Patient .....  
ID ..... DOB .....

Medicine/s	Amount (units)	÷	Volume (mL)	=	Conc (units/mL)
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....

Diluent .....  
Date ..... Prepared by .....  
Time ..... Checked by .....

JG1160

500/BOX

## For EPIDURAL Use Only

Patient .....  
ID ..... DOB .....

Medicine/s	Amount (units)	÷	Volume (mL)	=	Conc (units/mL)
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....

Diluent .....  
Date ..... Prepared by .....  
Time ..... Checked by .....

JG1168

500/BOX

## For EPIDURAL Use Only

Patient .....  
ID ..... DOB .....

Medicine/s	Amount (units)	÷	Volume (mL)	=	Conc (units/mL)
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....

Diluent .....  
Date ..... Prepared by .....  
Time ..... Checked by .....

JG1162

500/BOX

## For REGIONAL Use Only

Type .....  
Patient .....  
ID ..... DOB .....

Medicine/s	Amount (units)	÷	Volume (mL)	=	Conc (units/mL)
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....

Diluent .....  
Date ..... Prepared by .....  
Time ..... Checked by .....

JG1170

500/BOX

## For REGIONAL Use Only

Type .....  
Patient .....  
ID ..... DOB .....

Medicine/s	Amount (units)	÷	Volume (mL)	=	Conc (units/mL)
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....

Diluent .....  
Date ..... Prepared by .....  
Time ..... Checked by .....

JG1164

500/BOX

## REGIONAL REGIONAL

Catheter commenced: Date ...../...../.....  
Time .....

JG11785

500/BOX

## IntraTHECAL IntraTHECAL

Catheter commenced: Date ...../...../.....  
Time .....

JG11745

500/BOX

## EPIDURAL EPIDURAL

Catheter commenced: Date ...../...../.....  
Time .....

JG11765

500/BOX



# National Recommendation Labels

**For IntraVENOUS Use Only**

Patient .....  
 ID ..... DOB .....

Medicine/s	Amount (units)	÷	Volume (mL)	=	Conc (units/mL)
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....

Diluent .....  
 Date ..... Prepared by .....  
 Time ..... Checked by .....

JG1167

500/BOX

**For IntraVENOUS Use Only**

Patient .....  
 ID ..... DOB .....

Medicine/s	Amount (units)	÷	Volume (mL)	=	Conc (units/mL)
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....

Diluent .....  
 Date ..... Prepared by .....  
 Time ..... Checked by .....

JG1161

500/BOX

**For Subcutaneous Use Only**

Patient .....  
 ID ..... DOB .....

Medicine/s	Amount (units)	÷	Volume (mL)	=	Conc (units/mL)
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....

Diluent .....  
 Date ..... Prepared by .....  
 Time ..... Checked by .....

JG1169

500/BOX

**For Subcutaneous Use Only**

Patient .....  
 ID ..... DOB .....

Medicine/s	Amount (units)	÷	Volume (mL)	=	Conc (units/mL)
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....

Diluent .....  
 Date ..... Prepared by .....  
 Time ..... Checked by .....

JG1163

500/BOX

**ROUTE**

Patient .....  
 ID ..... DOB .....

Medicine/s	Amount (units)	÷	Volume (mL)	=	Conc (units/mL)
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....

Diluent .....  
 Date ..... Prepared by .....  
 Time ..... Checked by .....

JG1171

500/BOX

**ROUTE**

Patient .....  
 ID ..... DOB .....

Medicine/s	Amount (units)	÷	Volume (mL)	=	Conc (units/mL)
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....
.....	.....	.....	.....	.....	.....

Diluent .....  
 Date ..... Prepared by .....  
 Time ..... Checked by .....

JG1165

500/BOX

Route .....  
 Commenced: .....  
 Date ...../...../.....  
 Time .....

JG11815

500/BOX

**IntraVENOUS** | **IntraVENOUS**  
 Commenced: .....  
 Date ...../...../.....  
 Time .....

JG11755

500/BOX

**Subcutaneous** | **Subcutaneous**  
 Commenced: .....  
 Date ...../...../.....  
 Time .....

JG11795

500/BOX



# National Recommendation Labels

**For Intra-ARTERIAL Use Only**

Patient .....  
 ID ..... DOB .....

Medicine/s	Amount (units)	$\div$	Volume (mL)	$=$	Conc (units/mL)
.....	.....		.....		.....
.....	.....		.....		.....
.....	.....		.....		.....

Diluent .....  
 Date ..... Prepared by .....  
 Time ..... Checked by .....

JG1386

500/BOX

**For Intra-ARTERIAL Use Only**

Patient .....  
 ID ..... DOB .....

Medicine/s	Amount (units)	$\div$	Volume (mL)	$=$	Conc (units/mL)
.....	.....		.....		.....
.....	.....		.....		.....
.....	.....		.....		.....

Diluent .....  
 Date ..... Prepared by .....  
 Time ..... Checked by .....

JG1385

500/BOX

**For Enteral Use Only**

Patient .....  
 ID ..... DOB .....

Medicine/s	Amount (units)	$\div$	Volume (mL)	$=$	Conc (units/mL)
.....	.....		.....		.....
.....	.....		.....		.....
.....	.....		.....		.....

Diluent .....  
 Date ..... Prepared by .....  
 Time ..... Checked by .....

JG1672

500/BOX

**For Inhalation Use Only**

Patient .....  
 ID ..... DOB .....

Medicine/s	Amount (units)	$\div$	Volume (mL)	$=$	Conc (units/mL)
.....	.....		.....		.....
.....	.....		.....		.....
.....	.....		.....		.....

Diluent .....  
 Date ..... Prepared by .....  
 Time ..... Checked by .....

JG1987

500/BOX

**Burette Label for IntraVENOUS Use**

Patient .....  
 ID ..... DOB .....

Medicine/s	Amount (units)	$\div$	Volume (mL)	$=$	Conc (units/mL)
.....	.....		.....		.....
.....	.....		.....		.....
.....	.....		.....		.....

Date ..... Prepared by .....  
 Time ..... Checked by .....

JG1172

500/BOX

**Intra-ARTERIAL Intra-ARTERIAL**

Commenced: Date ...../...../.....  
 Time .....

JG11805

500/BOX

**Enteral Enteral**

Commenced: Date ...../...../.....  
 Time .....

JG16735

500/BOX

**CENTRAL VENOUS CENTRAL VENOUS**

Commenced: Date ...../...../.....  
 Time .....

JG11775

500/BOX

**Sodium Chloride 0.9%**

R74

500/BOX

Medicine .....

Conc (units/mL) .....

JG1173

500/BOX

**Medicine Medicine**

JG11825

500/BOX



# Jumbo Radiology Labels



JX0009 750/ROLL



JX0202 250/BOX



JX0203 250/BOX



JX0204 250/BOX

**NUCLEAR MEDICINE  
RADIO ACTIVE MATERIAL  
SKELETAL / BONE**

Dose \_\_\_\_\_ MBq Time \_\_\_\_\_  
Patient \_\_\_\_\_

JNM02 500/ROLL

**NUCLEAR MEDICINE  
RADIO ACTIVE MATERIAL  
LUNG**

Dose \_\_\_\_\_ MBq Time \_\_\_\_\_  
Patient \_\_\_\_\_

JNM03 500/ROLL

**NUCLEAR MEDICINE  
RADIO ACTIVE MATERIAL  
RENAL**


Dose \_\_\_\_\_ MBq Time \_\_\_\_\_  
Patient \_\_\_\_\_

JNM05 500/ROLL

**NUCLEAR MEDICINE  
RADIO ACTIVE MATERIAL**

Dose \_\_\_\_\_ MBq Time \_\_\_\_\_  
Patient \_\_\_\_\_

JNM07 500/ROLL

\_\_\_\_\_ 

ACTIVITY \_\_\_\_\_ VOL \_\_\_\_\_  
DATE \_\_\_\_\_ TIME \_\_\_\_\_

JNM08/R (REMOVABLE ADHESIVE) 500/ROLL

 **RADIOACTIVE  
MATERIAL**

JX0024 (REMOVABLE ADHESIVE) 500/ROLL

**DO NOT  
DESTROY**

JX0025 250/ROLL

**RADIOACTIVE MATERIAL**

Time: \_\_\_\_\_ Tracer: \_\_\_\_\_  
Activity: \_\_\_\_\_ Volume: \_\_\_\_\_  
Name: \_\_\_\_\_

JNM09 500/ROLL

**CONTRAST  
REACTION**

JX0028 500/ROLL

**DO NOT  
DESTROY**

BEFORE \_\_\_\_\_

JX0078 250/ROLL

**X-ray Contrast**

Contrast: \_\_\_\_\_  
Amount: \_\_\_\_\_  
Prescribed by: \_\_\_\_\_  
Checked by: \_\_\_\_\_  
Date: \_\_\_\_\_ Time: \_\_\_\_\_

JX0166 250/BOX

**DO NOT DESTROY  
FILE UNTIL**

\_\_\_\_\_

JX0237 500/BOX

**DUPLICATE**

JX0037 1000/BOX

**FILM TO:  
WARD / CLINIC**

JX0064 500/ROLL

**RADIOACTIVE**

JX0270 250/BOX




JX0077 250/BOX




# Alpha & Numerical Coding Labels




TSAAS 40/SHEET

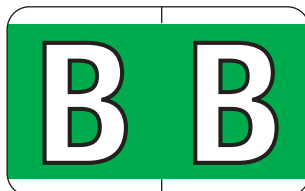

TSBBS 40/SHEET

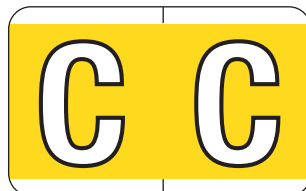


TSCCS 40/SHEET

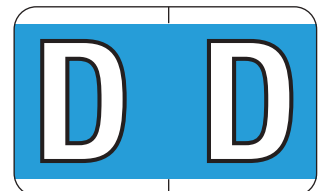

TSDDS 40/SHEET




TSEES 40/SHEET

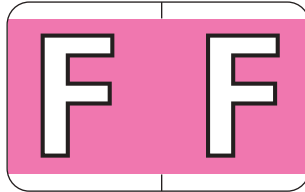


TSFFS 40/SHEET




TSGGS 40/SHEET

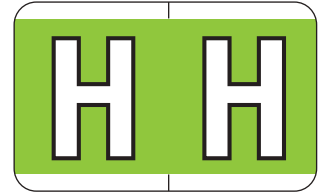

TSHHS 40/SHEET

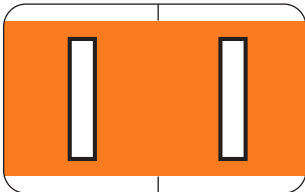

TSIIS 40/SHEET

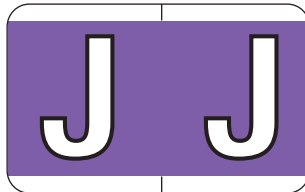

TSJJS 40/SHEET



TSKKS 40/SHEET



TSLLS 40/SHEET



TSMMS 40/SHEET



TSNNS 40/SHEET



TSOOS 40/SHEET



TSPPS 40/SHEET



TSQQS 40/SHEET



TSRRS 40/SHEET



TSSSS 40/SHEET



TS TTS 40/SHEET




TSUUS 40/SHEET



TSVVS 40/SHEET



TSWWS 40/SHEET

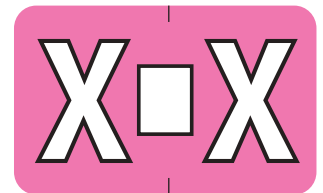

TSXXS 40/SHEET



TSYYS 40/SHEET



TSZZS 40/SHEET



TY22 500/ROLL



TY23 500/ROLL

TY LABELS - 40mm x 19mm, FIT THE TLD25 LABEL DISPENSER.  
CN LABELS - 32mm x 12mm, FIT THE TLD15 LABEL DISPENSER.



CN00 500/ROLL



CN01 500/ROLL



CN02 500/ROLL



CN03 500/ROLL



CN04 500/ROLL



CN05 500/ROLL



CN06 500/ROLL



CN07 500/ROLL



CN08 500/ROLL



CN09 500/ROLL



# Numerical Coding Labels



TL00 500/ROLL



TL11 500/ROLL



TL22 500/ROLL



TL33 500/ROLL



TL44 500/ROLL



TL55 500/ROLL



TL66 500/ROLL



TL77 500/ROLL



TL88 500/ROLL



TL99 500/ROLL




TS00 500/ROLL



TS11 500/ROLL




TS22 500/ROLL

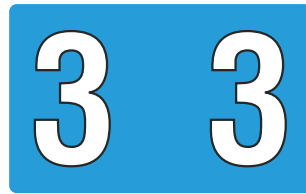

TS33 500/ROLL



TS44 500/ROLL

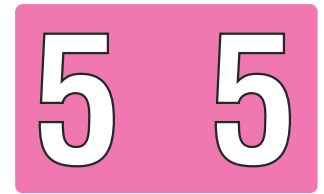

TS55 500/ROLL



TS66 500/ROLL



TS77 500/ROLL



TS88 500/ROLL



TS99 500/ROLL



JXB0 500/ROLL



JXB1 500/ROLL



JXB2 500/ROLL



JXB3 500/ROLL



JXB4 500/ROLL



JXB5 500/ROLL



JXB6 500/ROLL



JXB7 500/ROLL



JXB8 500/ROLL



JXB9 500/ROLL

TL LABELS - 40mm x 40mm, GLOSS PAPER.  
FIT THE TLD45 LABEL DISPENSER.

TS LABELS - 40MM X 25MM, LAMINATED &  
CENTRE CREASED.  
FIT THE TLD35 LABEL DISPENSER.

JXB LABELS - 20MM X 20MM, RADIANT RED.  
FIT THE TLD25 LABEL DISPENSER.



## TRIARC Specialises in Custom Printed Labels

We can design and make ANY kind of label to suit your particular requirements.


With our digital printing machines we can print any shape, size, colour or quantity at very cost effective prices.

## PHONE OR EMAIL YOUR REQUEST NOW FOR A QUOTE

PLEASE ADVISE US THE SIZE, TEXT COLOUR, BACKGROUND COLOUR AND QUANTITY.

We have over 1,000 cutting dies in many shapes and sizes.

Following are some of our standard sizes that we are regularly printing, but this is just a small selection of the sizes we have available.

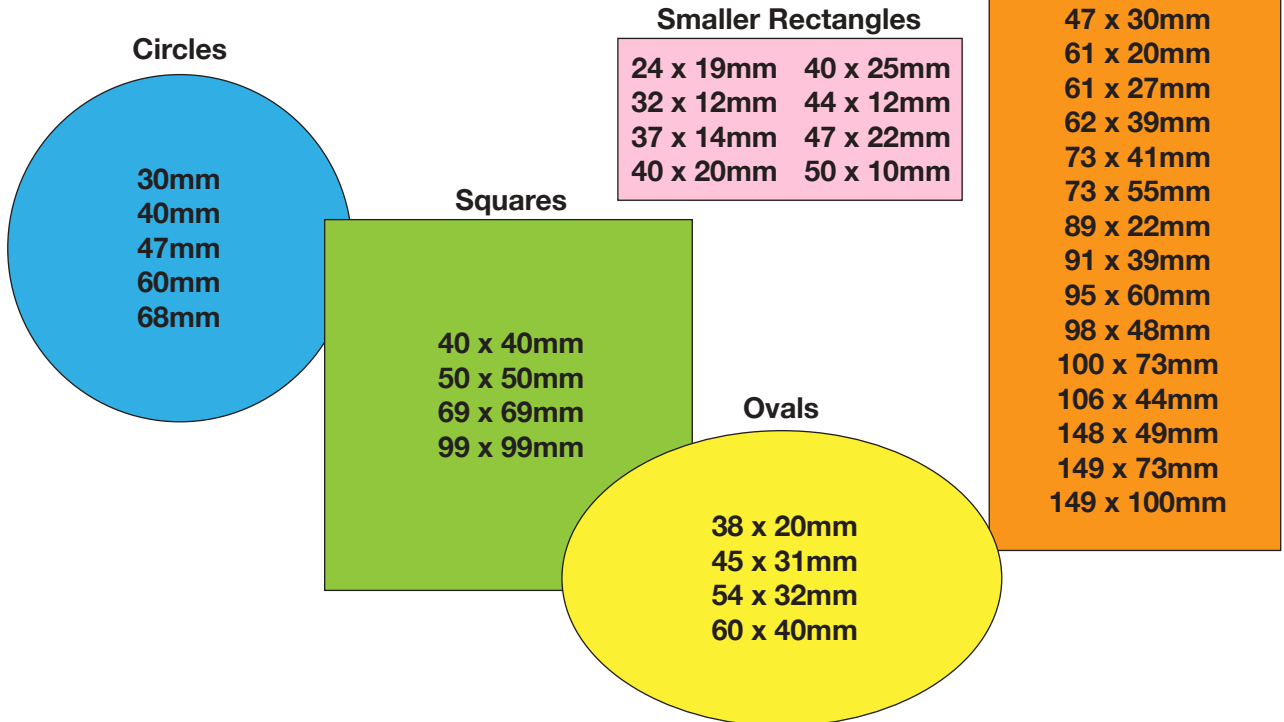

We can print onto a variety of materials such as Matt or Gloss Paper, Radiants / Fluoro's, Vinyls, Polypropylene, Polyester and other synthetic materials.

## Did you know that we can also do the following?

- Waterproof Labels
- Clear / Transparent Labels
- Barcoding
- Sequential Numbering
- Asset / Serial Coding
- Laminating

The above are excellent for labelling equipment where a durable label is needed which can withstand getting cleaned down regularly and is long lasting. You can also track your equipment by having a barcode or QR code on it.

- Thermal Transfer Ribbons
- Magnets
- Tags

**PLEASE CONTACT US FOR FURTHER INFORMATION ON THE ABOVE**